

# **Medical Robotics**

#### Dr. Gernot Kronreif

Mechatronic Automation Systems Austrian Research Centers Seibersdorf E-mail: gernot.kronreif@arcs.ac.at

2004 Summerschool, "Medical Robotics"

# Outline


Introduction to Robotics

- Terms and Definitions
- General Structure of a Robot System
- Medical Robotics Overview
- Selected Application Examples
- Summary and Outlook



ARCsr/WPA

Copyright © 2004, ARCsr/WPA

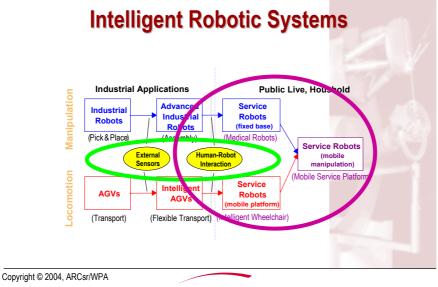

AUSTRIAN RESEARCH CENTERS SEIBERSDORF

2004 Summerschool, "Medical Robotics"

ARCsr/WPA

#### **Terms and Definitions**

#### Links and Joints


Links are the solid structural members of a robot, and joints are the movable couplings between them

#### Degree-of-Freedom (DOF)

Each joint on the robot introduces a degree of freedom. Each DOF can be a slider, rotary, or other type of actuator. Robots typically have 5 or 6 degrees of freedom. 3 of the degrees of freedom allow positioning in 3D space, while the other 2 or 3 are used for orientation of the end effector.

#### Work Envelope, Workspace

The work envelope is the boundary of positions in space that the robot can reach. The workspace is defined by the kinematic configuration of the robot (type of DOFs, orientation of joints) as well as by the ROM of each joint.

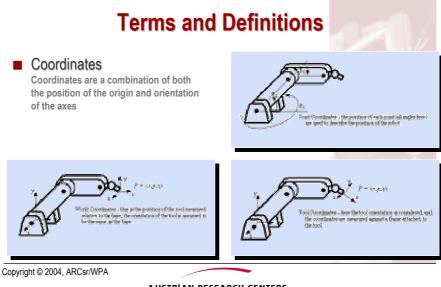

AUSTRIAN RESEARCH CENTERS

2004 Summerschool, "Medical Robotics"

ARCsr/WPA

#### **Terms and Definitions**

#### Accuracy

- "How close does the robot get to the desired point"
- This measures the distance between the specified position, and the actual position of the robot end effector.
- Accuracy is more important when performing off-line programming, because absolute coordinates are used.

#### Repeatability

- "How close will the robot be to the same position as the same move made before"
- A measure of the error or variability when repeatedly reaching for a single position.
- This is the result of random errors only
- Repeatability is often smaller than accuracy.

Copyright © 2004, ARCsr/WPA

#### **Terms and Definitions**

#### Accuracy and Repeatability are functions of ...

- Resolution the use of digital systems, and other factors mean that only a limited number of positions are available. Thus user input coordinates are often adjusted to the nearest discrete position.
- Kinematic modeling error the kinematic model of the robot does not exactly match the robot. As a result the calculations of required joint angles contain a small error.
- Calibration errors The position determined during calibration may be off slightly, resulting in an error in calculated position.
- Random errors problems arise as the robot operates. For example, friction, structural bending, thermal expansion, backlash/slip in transmissions, etc. can cause variations in position.

Copyright © 2004, ARCsr/WPA

AUSTRIAN RESEARCH CENTERS

2004 Summerschool, "Medical Robotics"

ARCsr/WPA

#### Main Components of a Robot System

Mechanical structure (links, base, etc).

Required mass to provide enough structural rigidity to ensure minimum accuracy under varied payloads.

Actuators


Motors, cylinders, etc. that drive the robot joints. This might also include mechanisms for a transmission, locking, etc.

- Main Controller This computer interfaces with the user, and in turn controls the robot joints.
- Effector, "End of Arm Tooling"

Designed for specific tasks.

Handheld Operation Unit, "Teach pendant"


Popular method for programming the robot. Small hand held device that can direct motion of the robot, record points in motion sequences, and begin replay of sequences.

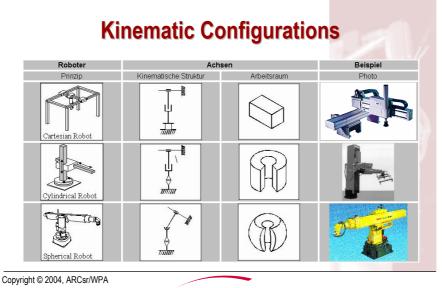

AUSTRIAN RESEARCH CENTERS

2004 Summerschool, "Medical Robotics"

ARCsr/WPA

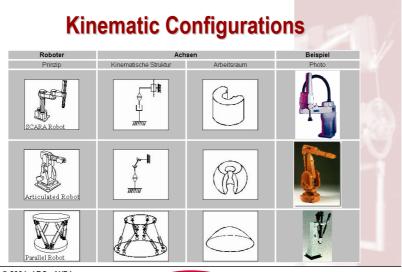

Copyright © 2004, ARCsr/WPA

#### **Special Configurations for Medical Robotics**



Copyright © 2004, ARCsr/WPA

AUSTRIAN RESEARCH CENTERS SEIBERSDORF


2004 Summerschool, "Medical Robotics"


ARCsr/WPA

#### Serial vs. Parallel Kinematik Chain? Eigenschaften Nutzlast / Gewicht 1:10 bis 1:20 1:1 bis 1:2 Kin. Struktur anthropomorph kompakt Steifigkeit hoch gering Intraoperatives schwierig einfach Handling Arbeitsbereich groß klein Genauigkeit gering hoch Positionsfehler akkumuliert gemittelt Technische Komplexität groß gering Verhalten in große Bewegungen große Kräfte Singularität große Beschleunigungen

Copyright © 2004, ARCsr/WPA



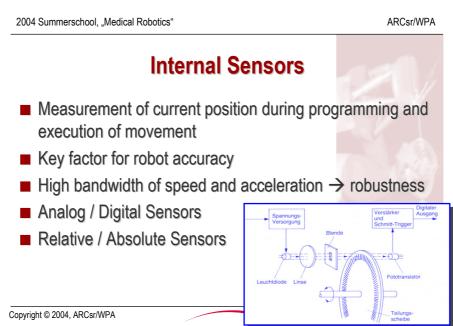

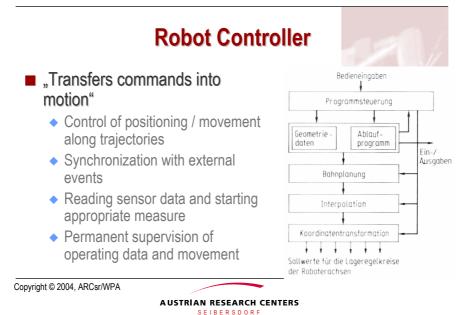

2004 Summerschool, "Medical Robotics"

ARCsr/WPA

#### **Controller Hardware**

- CPU
  - 16-bit or 32-bit micro-processor; arithmetic co-processor for trigonometric calculations
- Memory Unit
- Position Control Modules
  - Control of position/velocity
- I/O Components
  - Exchange of information with auxiliary devices; serial/parallel interface; DI/DO cards; networks (field bus, LAN)
- Power Supply
- Teach Panel, Handheld Control Unit

Copyright © 2004, ARCsr/WPA

ARCsr/WPA



Copyright © 2004, ARCsr/WPA

AUSTRIAN RESEARCH CENTERS

2004 Summerschool, "Medical Robotics"

ARCsr/WPA

# Safety Regulations IR (EN 775)

#### Sources of Risks:

- Loss/Malfunction at safety system, energy supply, control system, etc.
- Moving mechanical components leading to contusion
- Stored energy
- Energy source
- Human failure

at design and/or realization, putting into operation, functional check, operation, programming and testing, maintenance


Copyright © 2004, ARCsr/WPA

# Safety Regulations IR (EN 775) Safety Measurements Safety zones Safety zones Limitation by means of hardware stops or similar measurements Reduced velocity Fences, etc. Emergency Stop Safety measurements must be "FAIL SAVE"

AUSTRIAN RESEARCH CENTERS


2004 Summerschool, "Medical Robotics"

ARCsr/WPA

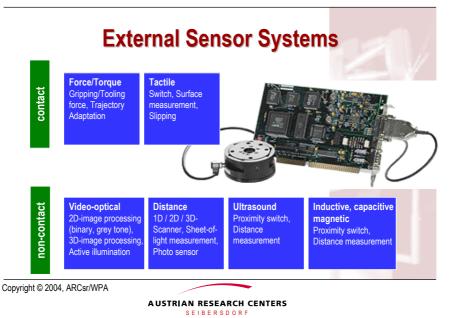

#### Industrial robots for medical Applications?

- Major design criteria IR: Working envelope û, Velocity û
- SEVERE modifications for system safety (not only SW!)
- Application Example: Orthopedics, Radiation Therapy



Copyright © 2004, ARCsr/WPA

AUSTRIAN RESEARCH CENTERS

2004 Summerschool, "Medical Robotics"

ARCsr/WPA

# ➔ special design for medical Applications!

- Major design criteria : SAFETY ☆
- Velocity, working envelope ♣
- Special kinematic designs ("mechanical constraints")



Copyright © 2004, ARCsr/WPA

#### Problems to be solved .... Mechanical Design Design for ACCURACY rather than repeatability "Shared Control" → backdrivable robot systems Sterilization Compatibility to intra-operative imaging!!!!! Accessibility Sensors, Control Master-Slave New advanced sensor systems (nano-sensors) !!!!! "Shared Control", automation of routine operations (e.g. suturing) (active) compensation of tissue movement (models for tool/tissue interaction) "Visual servoing" Copyright © 2004, ARCsr/WPA **AUSTRIAN RESEARCH CENTERS** SEIBERSDORF

2004 Summerschool, "Medical Robotics"

ARCsr/WPA

# <section-header> Bedie Bedi

Copyright © 2004, ARCsr/WPA

# **Medical Robotics - Applications**

#### Robots for Rehabilitation: Providing handicapped people higher degree of autonomy and mobility. "Assistive Devices". Stationary robot systems (simple handling tasks) and/or mobile robot systems (autonomous wheelchair). Robot for post-stroke therapy!!! Robots for Diagnosis/Therapy, "OR-Robots": Assistance during surgical intervention - (more or less) guided by robot control; PROs: precision, reliability, time reduction; CONs: extensive planning, costs

Copyright © 2004, ARCsr/WPA

AUSTRIAN RESEARCH CENTERS

2004 Summerschool, "Medical Robotics"

#### ARCsr/WPA

#### **Types of Interaction**

Autonomous Procedures

• Examples: THR/TKR, radiation therapy

#### Interactive / Robot"assistant"

- Robot and surgeon "share" control ("shared control")
- "Hands-on" systems, "active constraints"-methods
- Examples: Milling and/or cutting procedures in orthopaedics

#### Explicit control by surgeon ("Master-Slave")

- Supporting at minimal-invasive interventions
- "Tele-Operation", "Tele-Presence"

Copyright © 2004, ARCsr/WPA

## **Robots for Autonomous Procedures**

- Once positioned by a surgeon, robot removes tissue automatically
- Lack of direct surgeon involvement
- Problems with intra-operative tissue motion
- Examples: ROBODOC, CASPAR, CyberKnife



Copyright © 2004, ARCsr/WPA

#### AUSTRIAN RESEARCH CENTERS

2004 Summerschool, "Medical Robotics"

ARCsr/WPA

## "Hands-On" - Systems

- Force controlled joystick on end of robot; Surgeon moves joystick, back-driving under servo- assist
- Robot constrains within a pre-op plan: Surgeon judges, senses, adapts a good synergy
- Special requirements for robot design (low impedance, no brakes, back-drivable, etc.)
- New type of surgery robot
- Example: "ACROBOT"



Copyright © 2004, ARCsr/WPA

#### Master/Slave - Telemanipulation

- Generally Master near to patient in O. R. but not "hands- on"
- Generally little tactile information
- Uses high quality imaging
- Motion scaling of Master to Slave is possible
- Examples: Zeus, daVinci


Copyright © 2004, ARCsr/WPA



AUSTRIAN RESEARCH CENTERS SEIBERSDORF

2004 Summerschool, "Medical Robotics"

ARCsr/WPA

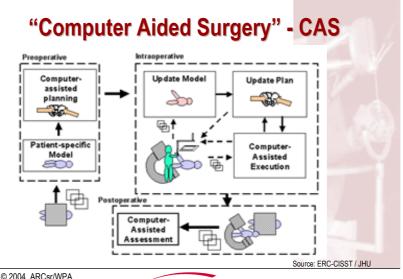

Copyright © 2004, ARCsr/WPA

## Surgical CAD/CAM

#### "Surgical CAD"

is analogous to computer-aided design in manufacturing systems. Preoperatively, medical images, anatomical atlases, and other information are combined to make a model of an individual patient. The computer then assists the surgeon in planning and optimizing an appropriate intervention.

#### "Surgical CAM"

is analogous to computer-aided manufacturing. The data from the preoperative planning step (images, models, plan geometry, etc.) is all brought into the operating room. Real time images and other sensor data are used to "register" the preoperative plan to the actual patient, and the model and the plan are updated throughout the procedure. The actual surgical procedure is performed by the surgeon with the assistance of the computer.

#### "Surgical TQM"

is analogous to "total quality management" in manufacturing, and reflects the important role that the computer can play in reducing surgical errors and in promoting more consistent and improved outcomes. It is built into the entire process.

Copyright © 2004, ARCsr/WPA

AUSTRIAN RESEARCH CENTERS

2004 Summerschool, "Medical Robotics"

ARCsr/WPA

#### Medical Robotics vs. "Augmented Reality"

- Why to use a robot? Is "Augmented Reality" a better choice?
- Are there any advantages from the use of a robot which justify the higher cost / complexity?
- Who is in charge?
- Clinical acceptance?



Copyright © 2004, ARCsr/WPA

AUSTRIAN RESEARCH CENTERS SEIBERSDORF

# **Clinical Applications**

#### Neurosurgery

- Frameless stereotactic applications → high spatial accuracy and precise targeting
- Orthopedic Surgery
  - THR, TKR, spine interventions → autonomous procedures due to rigid nature of bone
- General and Thoracic Surgery
  - Camera holder for laparoscopic surgery
  - Active instruments
  - Percutaneous interventions

Copyright © 2004, ARCsr/WPA



2004 Summerschool, "Medical Robotics"

ARCsr/WPA

#### PathFinder: Armstrong Healthcare, Ltd.

- Precise "localizer" for neurosurgery positioning of surgical instruments along pre-defined trajectory
- Removes the need for a stereotactic frame and its associated calculations; robot serving as a precision tool localizer
- Head supported by standard Mayfield clamp during surgery, in any convenient position
- Automatic registration of images and patient
- DICOM3 Interface for CT und MR data

# PathFinder: Armstrong Healthcare, Ltd.





Copyright © 2004, ARCsr/WPA

AUSTRIAN RESEARCH CENTERS

2004 Summerschool, "Medical Robotics"

ARCsr/WPA

## ROBODOC: Integrated Surgical Systems Inc.



 Components: Planning workstation (OrthoDOC), robot, control system


■ Target: Cementless implantation → natural bone growth into implant → long-term improvement of implant fit

Robotic system for precise cutting of the femoral cavity



Copyright © 2004, ARCsr/WPA

ARCsr/WPA

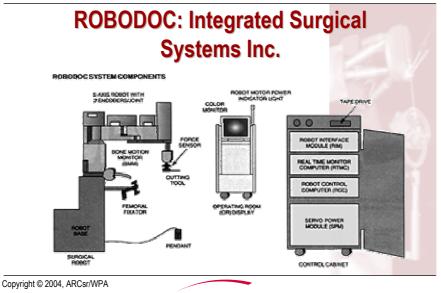

AUSTRIAN RESEARCH CENTERS

2004 Summerschool, "Medical Robotics"

ARCsr/WPA

# ROBODOC: Integrated Surgical Systems Inc.

- Implanting of three locator pins in hip
- CT scan → transfer to OrthoDOC
- Planning of the implant (size, position, etc.)
- Calculation of the cutting procedure → transfer to robot controller
- Exposing hip joint
- Registration robot patient
- Autonomous cutting; surgeon monitors process



Copyright © 2004, ARCsr/WPA

# Laparoscopic Surgery -- Problems

MIS: advantages for patient, but challenge for surgeon


- Working with long instruments via small incisions
- Incision acting as pivot point for tools
- Reduced degrees-of freedom → limited dexterity
- Variable scaling of movement
- Unnatural hand-eye coordination (mirrored movements)
- No real 3D-vision
- No (bad) tactile feedback

Copyright © 2004, ARCsr/WPA



2004 Summerschool, "Medical Robotics"

ARCsr/WPA

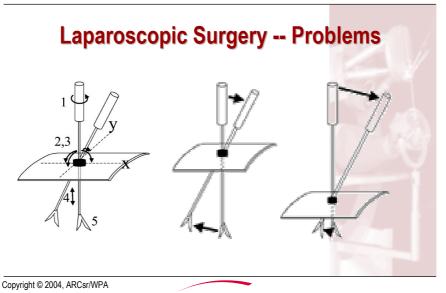

# AESOP (Automated Endoscopic System for Optimal Positioning) Computer Motion Inc. Speech-controlled robot serving as camera holder Fast, easy setup at OR (about 5 minutes) 23 commands available Additional robot control: Hand- and footswitch Storing/Restoring of particular positions

AUSTRIAN RESEARCH CENTERS


2004 Summerschool, "Medical Robotics"

ARCsr/WPA

# daVinci: Intuitive Surgical, Inc.

- Master-slave system for minimally invasive surgery
- Initial clinical application: cardiac surgery
- Components: Surgeon's console, control unit, three-arm surgical robot
- High resolution 3D image for surgeon
- Additional DOF at surgical instruments ("EndoWrist")
- "Motion scaling", tremor filter, "Indexing"
- Current research: Force-Feedback

# daVinci: Intuitive Surgical, Inc.

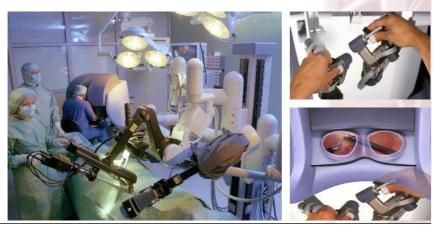

Copyright © 2004, ARCsr/WPA

AUSTRIAN RESEARCH CENTERS SEIBERSDORF

2004 Summerschool, "Medical Robotics"

ARCsr/WPA

#### "B-Rob I" – Percutaneous Interventions

- 4-DOF gross positioning stage
- 3-DOF fine positioning stage for secure and precise needle angulation
- Robot control system with dedicated safety features
- Dedicated hardware interface "UI"
- Navigational software "ROBUST" to define needle trajectory and to monitor robot position during intervention
- Optical tracker (NDI Polaris<sup>™</sup>)

# **CT-guided Bx Procedure - Setup**



Copyright © 2004, ARCsr/WPA

AUSTRIAN RESEARCH CENTERS SEIBERSDORF

2004 Summerschool, "Medical Robotics"

ARCsr/WPA

### New Development – "B-Rob II"



Copyright © 2004, ARCsr/WPA

# Safety of Medical Robot Systems

#### Compared to IR Systems ...

#### People (patient, physician) INSIDE working area of robot

- Additional REDUNDANT sensor systems
- Design of special purpose robot systems (mechanical constraints)
- Adequate, customized functionality of the robot system
- Fail-save techniques
- Sterilization, infection control!!
- USER INTERFACE!!!!!!

Non-generic applications
 TESTS, SIMULATION

Copyright © 2004, ARCsr/WPA



2004 Summerschool, "Medical Robotics"

ARCsr/WPA

# **Medical Robotics - Disadvantages**

- Solution More costly / complex than alternatives, e.g. Computer Aided Surgery
- ⊗ Is the robot safe?
- 8 Who is in charge?
- Not able to make own decisions
- Eimited flexibility
- (Currently) not able to deal with intra-operative tissue movement





#### **Medical Robotics - Advantages**

- More accurate than manual (esp. complex trajectories and/or exact positioning in 3D)
- Minimally invasive
- Solution Robot guides / constrains (safer?)
- Consistent quality
- Sepetitive motions without tiring
- History of motions recorded
- Small movements with small forces (scaling)
- ☺ "Indexing"
- © Sterilisation, resistant against germs/radiation etc.

Copyright © 2004, ARCsr/WPA

#### AUSTRIAN RESEARCH CENTERS SEIBERSDORF

2004 Summerschool, "Medical Robotics"

ARCsr/WPA

# Major Acceptance Issue

Robots will be successful ONLY if they

# → improve patient outcome, → lower cost, → or both!!!